

(12) **UK Patent Application** (19) **GB** (11) **2 379 610** (13) **A**

(43) Date of A Publication 19.03.2003

(21) Application No 0216145.3

(22) Date of Filing 12.07.2002

(30) Priority Data

(31) 0120645

(32) 24.08.2001

(33) GB

(51) INT CL<sup>7</sup>

A61L 29/00 31/10 31/18 , A61M 25/01

(52) UK CL (Edition V )

A5R RGEX

C3L LFG

(71) Applicant(s)

Smiths Group Plc

(Incorporated in the United Kingdom)

765 Finchley Road, LONDON, NW11 8DS,  
United Kingdom

(56) Documents Cited

EP 0624342 A1

EP 0386936 A1

WO 1998/019713 A1

DE 004014998 A1

DE 003936162 A1

WPI Abstract Accession No.1987-121289/17 of  
SU 1255450 A1 (KZEN-R KAZAN)

(72) Inventor(s)

Stephen James Field

(58) Field of Search

INT CL<sup>7</sup> A61B, A61L, A61M

Other: ONLINE : EPODOC, WPI, JAPIO

(74) Agent and/or Address for Service

J M Flint


765 Finchley Road, LONDON, NW11 8DS,  
United Kingdom

(54) Abstract Title

**PLASTIC CATHETER WITH ENHANCED ULTRASOUND VISIBILITY**

(57) An embryo replacement catheter has a flexible extruded shaft 1 of a transparent polyurethane with a bore 10 extending along its length. Gas bubbles 12 of a diameter in the range 5 $\mu$  to 10 $\mu$  are incorporated into the thickness of the wall of the shaft by adding gas during extrusion. The bubbles 12 are selected to increase the visibility of the catheter under ultrasound imaging whilst still enabling material flowing along the catheter to be seen.

**Fig.2.**

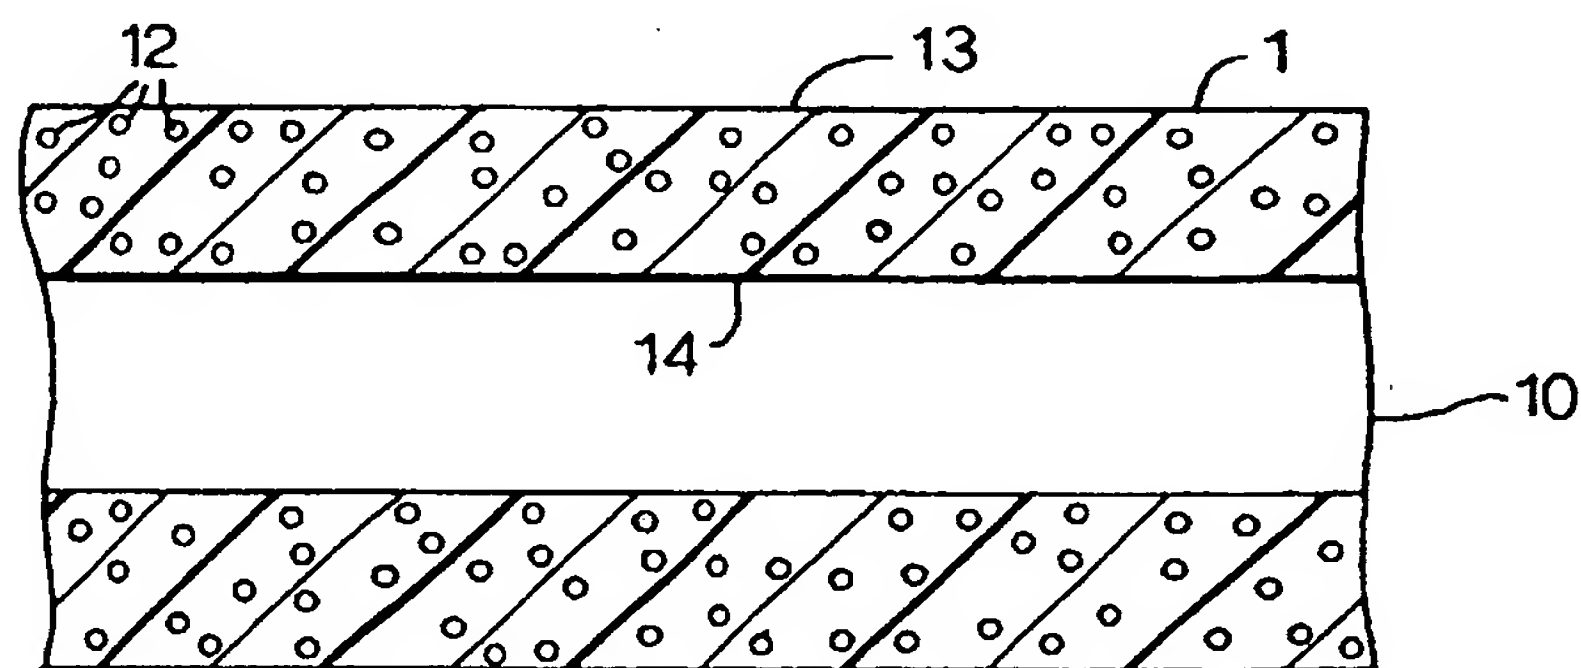

**GB 2 379 610 A**

1/1

Fig.1

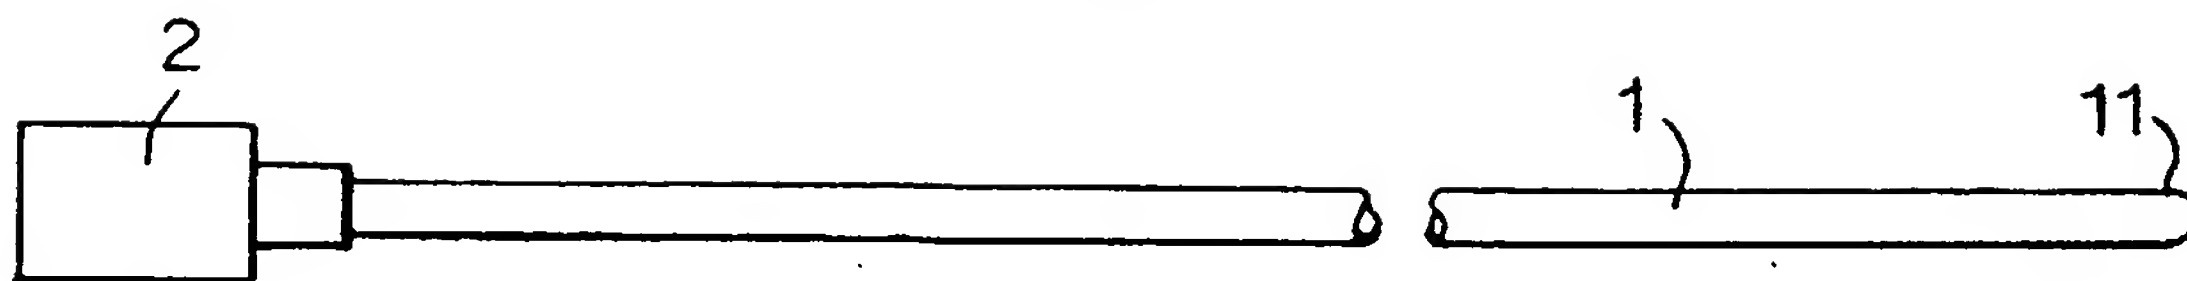


Fig.2.

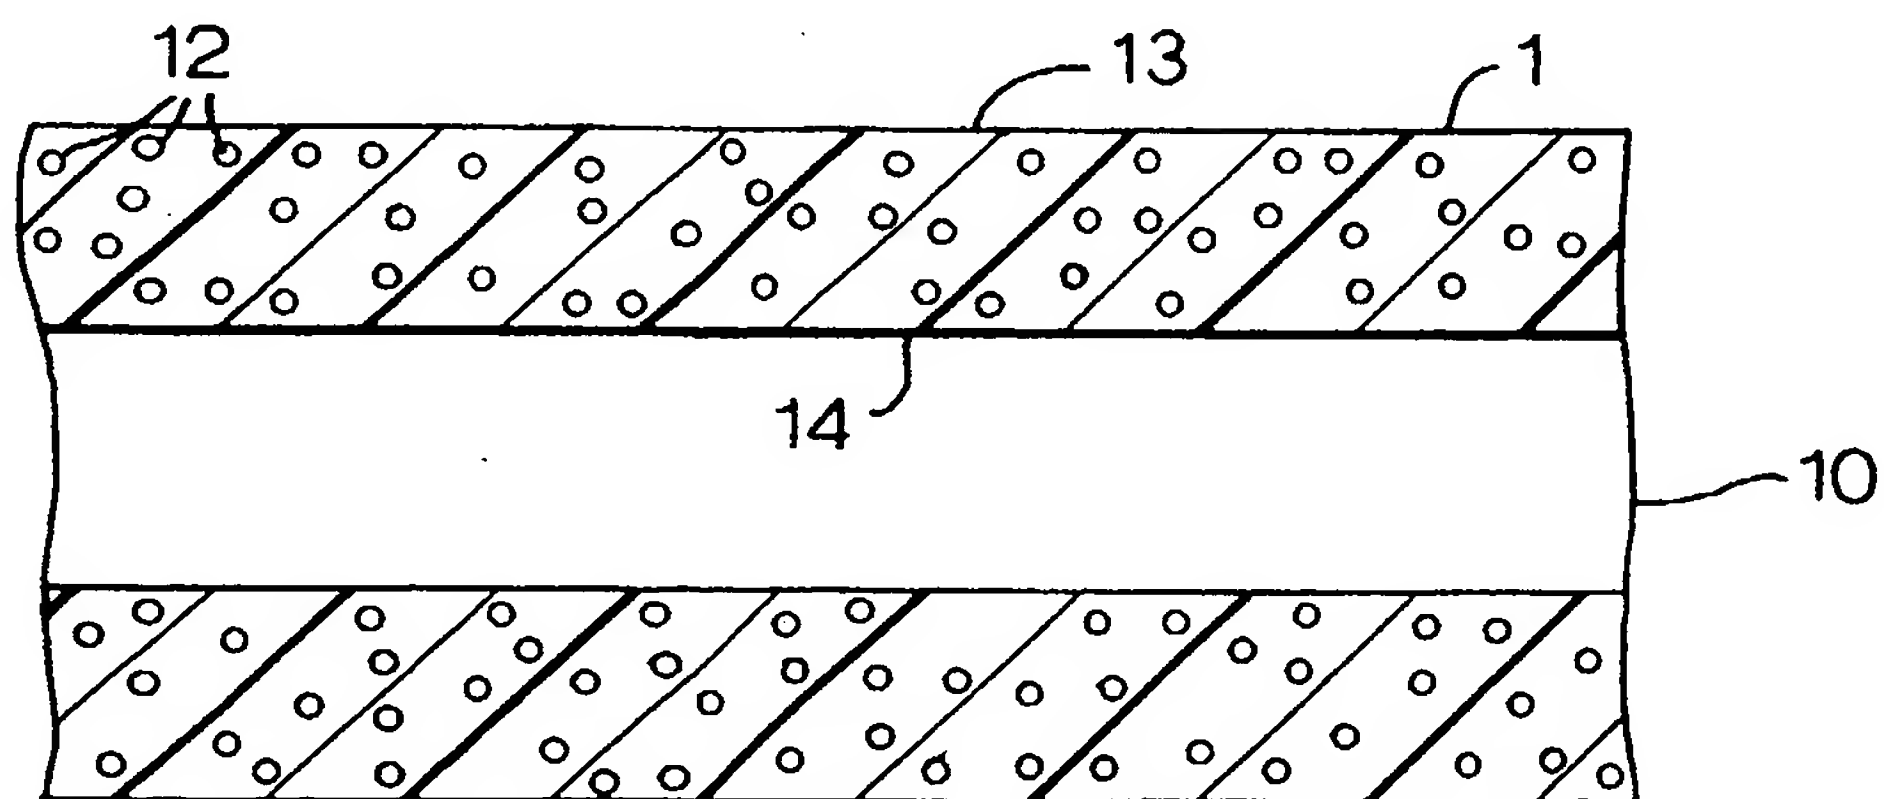


Fig.3.


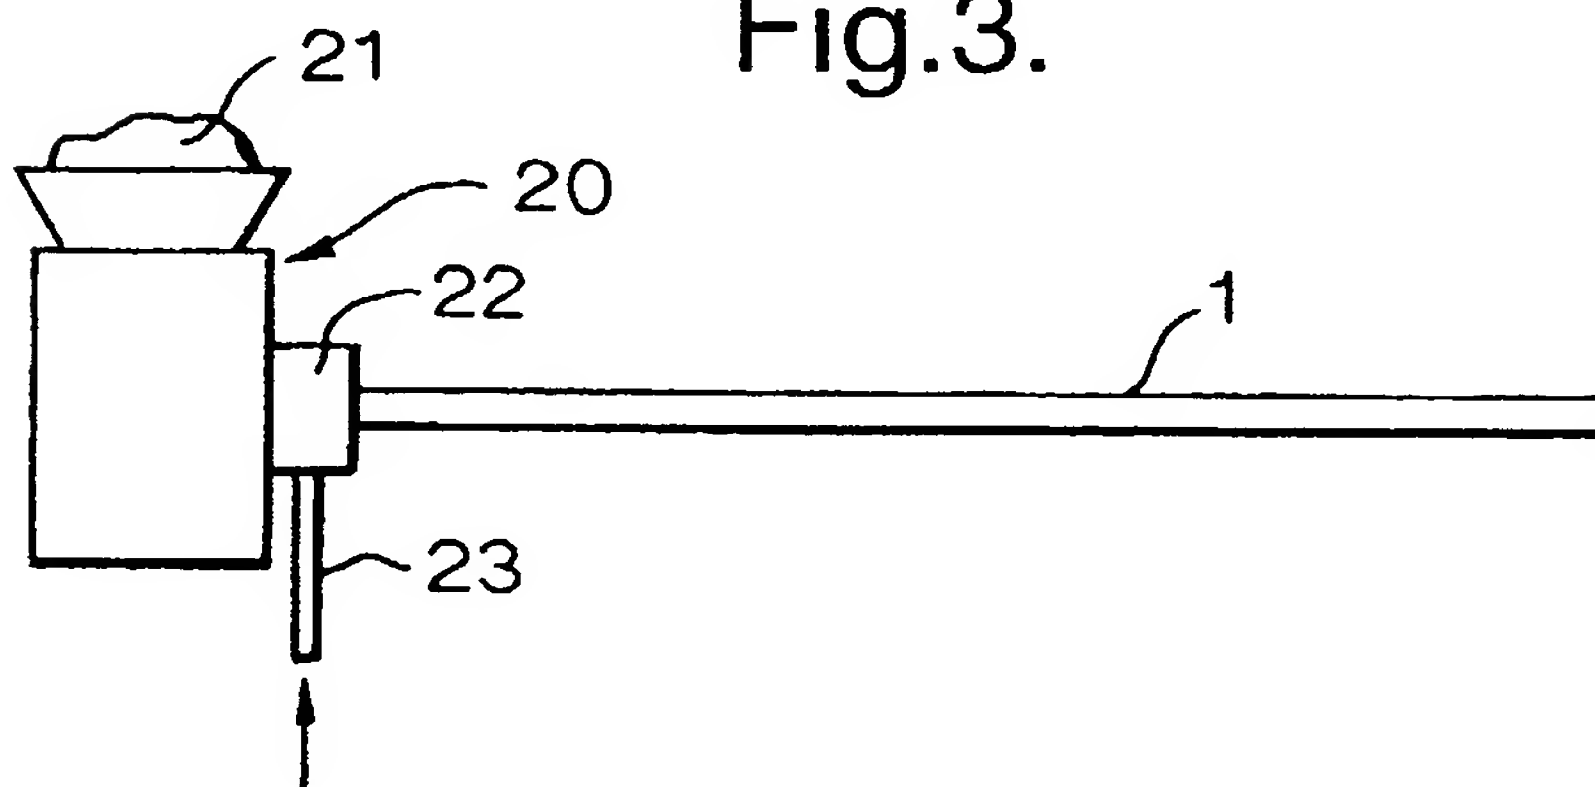


Fig.4.

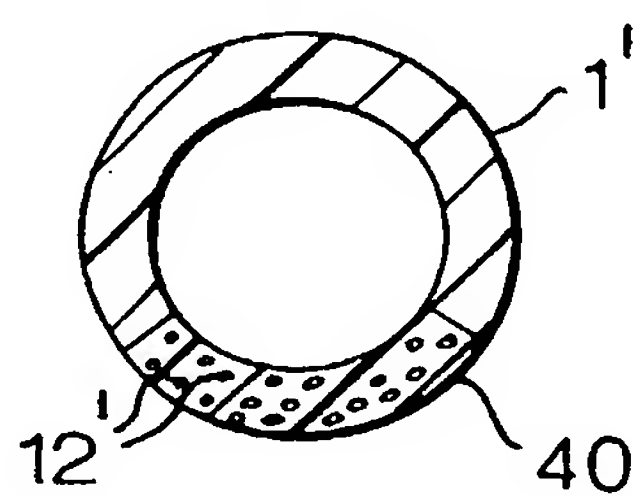

## MEDICO-SURGICAL DEVICES

This invention relates to medico-surgical devices.

The invention is more particularly concerned with medico-surgical devices, such as catheters, that are visible under ultrasound observation.

Ultrasound imaging equipment is increasingly being used during surgical procedures to monitor the location of a device within the body. The visibility of a device under ultrasound depends on various factors including the difference between the acoustic impedance of the material of the device and that of the surrounding medium, such as the patient tissue or body fluid within which the device is located. This difference is relatively low with plastic devices such as catheters and may make conventional catheters difficult to locate. Even devices of metal, such as needles, present problems of visibility under ultrasound observation because of the directional nature of the reflections. In some orientations a metal needle may be clearly visible but in other orientations it may be considerably less visible.

Attempts have been made to increase the visibility of medico-surgical devices under ultrasound observation in various ways. The surface of the device may be modified, such as by forming grooves or indentations in its surface. A reflective coating may be applied to the device, such as incorporating bubbles, as described in WO98/19713 and EP0624342. Alternatively, a metal marker may be secured to a plastics catheter.

It is an object of the present invention to provide an alternative medico-surgical device.

According to one aspect of the present invention there is provided a medico-surgical device of a plastics material, the material including gas bubbles through the major part of the thickness of the material in at least a part of the device such as to increase the visibility of the device under ultrasound imaging.

The device is preferably tubular and the gas bubbles may be provided around the entire circumference of the device or may be provided in a region of the device occupying only a part of the circumference of the device, such as a strip extending along the length of the device. The outer surface of the device may be smooth and uninterrupted by gas bubbles, and the device may have an inner surface that is smooth and uninterrupted by gas bubbles. The bubbles may have a diameter in the range  $1\mu$  to  $50\mu$  and preferably have a diameter in the range  $5\mu$  to  $10\mu$ . The bubbles may be substantially spherical. The device may be extruded, the gas bubbles being formed by addition of gas during extrusion of the device. Alternatively, the gas bubbles may be formed by a chemical foaming agent or by the incorporation of hollow microspheres into the plastics material. The plastics material is preferably substantially transparent, the size and density of the bubbles being selected such as to enable material flowing along the device to be viewed by the eye. The plastics material may be polyurethane.

According to another aspect of the present invention there is provided an embryo replacement catheter comprising a flexible, hollow, extruded shaft of a substantially

transparent plastics material, the shaft including gas bubbles through the thickness of its wall, the density and size of the bubbles being selected to increase visibility of the catheter under ultrasound imaging whilst enabling an embryo within the catheter to be viewed by the eye, and the bore of the catheter being smooth and uninterrupted by the gas bubbles.

According to a third aspect of the present invention there is provided a method of making a medico-surgical device comprising the steps of extruding a plastics material while incorporating a gas into the wall of the device such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.

According to a fourth aspect of the present invention there is provided a method of making a medico-surgical device comprising forming a wall of a plastics material containing a chemical foaming agent such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.

According to a fifth aspect of the present invention there is provided a method of making a medico-surgical device comprising forming a wall of a plastics material containing hollow microspheres such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.

According to a sixth aspect of the present invention there is provided a device made by a method according to the above third, fourth or fifth aspect of the present invention.

An embryo-transfer catheter and its method of manufacture, according to the present invention, will now be described, by way of example, with reference to the accompanying drawing, in which:

Figure 1 is a side elevation view of the catheter;

Figure 2 is a sectional side elevation view of a part of the catheter of Figure 1 to a larger scale;

Figure 3 illustrates schematically manufacture of the catheter; and

Figure 4 is a sectional transverse view through an alternative catheter.

- With reference first to Figures 1 and 2, the catheter comprises a flexible shaft 1 and a hub 2 joined at the rear end of the shaft. The shaft 1 has a circular section and a bore 10 extending along its length. The shaft 1 opens at its forward, right-hand, patient end 11, which is atraumatically rounded. The shaft 1 is extruded from a clear, transparent polyurethane material and incorporates small, gas-filled bubbles 12 the size and distribution of which are selected to increase the visibility of the catheter under ultrasound observation. Typically, the gas bubbles have a diameter in the range of about  $0.1\mu$  to  $300\mu$ , preferably being between  $1\mu$  and  $50\mu$  with the most preferred range being  $5\mu$  to  $10\mu$ . The bubbles 12 extend through the

entire thickness of the wall of the shaft 1 and may be spherical or of any other regular or irregular shape. The outer and inner surfaces 13 and 14 of the shaft may be smooth and uninterrupted by gas bubbles or the bubbles may break the surface.

The hub 2 serves to make connection with the shaft 1 and is moulded from a rigid, transparent plastics material, being subsequently bonded with the rear end of the shaft.

The shaft 1 is extruded in the manner shown in Figure 3 using an extrusion machine 20. Polyurethane material 21 is heated and supplied to the extrusion head 22 in the usual way but a gas such as nitrogen or carbon dioxide is also injected through the inlet 23 under pressure into the melt. As the plastics emerges from the extrusion head 22 the gas expands to form the bubbles 12. The relatively gas-permeable nature of the plastics means that after manufacture the bubble-forming gas will quickly escape and be replaced with air.

The shaft 1 can be extruded continuously at low cost, without the need for any subsequent operations apart from attaching the hub 2 and end forming the patient end tip 11.

The catheter shaft could be formed by other melt processes, such as injection moulding or blow moulding.

The bubbles could be formed in ways other than by injection of gas into the melt. For example, chemical foaming agents could be added to the plastics material, such as: azocarbonomides, dinitrosopentamethylene-tetramine, benzenephonohydrazine, 4,4 oxybis(benzenephonohydrazine), NN<sup>1</sup>dimethyl-NN<sup>1</sup> dinitrosoterephthalamide,



azoisobutyronitrile, sodium bicarbonate, terephthalazide or trihydrazinatrazine. Another way of forming the gas bubbles would be by incorporating a liquid into the plastics melt which volatises during the melt process. Alternatively, solid powdered dry ice (carbon dioxide) could be incorporated into the melt so that the particles of dry ice become gas bubbles during the forming process. It might be possible to use other solids which undergo sublimation in this way. The bubbles could be formed directly as a result of chemical reaction during polymerisation and or alternatively during cross-linking. The bubbles could be formed mechanically by whipping the plastics in a liquid form, such as in the manner used to form latex foam. The bubbles could be formed by the incorporation of hollow microspheres of resin or glass. Alternatively, small particles of a soluble material could be added to the plastics melt and subsequently dissolved away.

A shaft of this kind can have good visibility under ultrasound imaging without producing multiple echoes and can produce a good image regardless of the orientation of the shaft. The shaft can be made sufficiently transparent to ultrasound energy to enable material flowing along the bore of the catheter to be observed on the ultrasound image.

Because the catheter does not require any coating or separate marker there is no need for subsequent assembly operations and there is no risk of detachment. The catheter can be made of conventional medically-approved materials so does not present any new risk to the patient. Because the surface of the catheter can be smooth, the catheter can be inserted or slid through an outer tube with low friction. The smooth bore of the catheter ensures free flow along the bore, which can be important where the catheter is used to transfer embryos. The smooth surfaces also reduce the accumulation of biofilm on the catheter. The catheter can be



made without the need for metal components, which can be an advantage where the catheter is used while the patient is being viewed by magnetic imaging techniques. The catheter can be completely transparent to x-rays or the plastics from which it is formed could incorporate an x-ray opaque filler, such as barium sulphate.

The bubble size and density can be selected so that the optical transparency of the plastics forming the shaft remains sufficient to enable material flowing along the shaft to be viewed by the eye.

There are various ways in which the catheter could be modified. For example, it could be preferable for the bubbles to have a non-spherical shape and be oriented in a particular direction, such as longitudinally. This could be achieved by means of an obstruction in the extrusion die that constricts and elongates the bubbles as they flow through. Such an arrangement may give an increase in ultrasound visibility whilst reducing the opacity of the shaft to the eye.

It is not essential for the bubbles to be provided around the entire circumference of the shaft. As shown in Figure 4, the bubbles 12' could be formed only in one or more stripes extending along the shaft 1', such as in the stripe 40. This arrangement can be used where the shaft needs to have increased clarity so that material within the catheter can be seen by the eye. The bubble region need not be continuous along the length of the catheter. Instead, discrete separate regions with bubbles could be separated from one another along the length of the catheter by regions without bubbles. A shaft for such a catheter could be made by interrupting gas flow to the extruder. Where the bubbles are contained within a stripe, this

could be interrupted to make it discontinuous by extruding the stripe using two auxiliary extruders, one having material with a blowing agent and the other having material without the blowing agent. Alternate extruders are switched on and off so that the stripe can have sections containing bubbles separated from one another by sections without bubbles. A catheter with an interrupted bubble region may give a clearer ultrasound indication of movement of the catheter along its length and may also enable clearer observation of material flowing along the catheter both by ultrasound and by the eye.

CLAIMS

1. A medico-surgical device of a plastics material, wherein the material includes gas bubbles through the major part of the thickness of the material in at least a part of the device such as to increase the visibility of the device under ultrasound imaging.
2. A device according to Claim 1, wherein the device is tubular.
3. A device according to Claim 1 or 2, wherein the gas bubbles are provided around the entire circumference of the device.
4. A device according to Claim 1 or 2, wherein the gas bubbles are provided in a region of the device occupying only a part of the circumference of the device.
5. A device according to Claim 4, wherein the region is a strip extending along the length of the device.
6. A device according to any one of the preceding claims, wherein the outer surface of the device is smooth and uninterrupted by the gas bubbles.
7. A device according to any one of the preceding claims, wherein the device has an inner surface and the inner surface is smooth and uninterrupted by the gas bubbles.

8. A device according to any one of the preceding claims, wherein the bubbles have a diameter in the range  $1\mu$  to  $50\mu$ .
9. A device according to Claim 8, wherein the bubbles have a diameter in the range  $5\mu$  to  $10\mu$ .
10. A device according to any one of the preceding claims, wherein the bubbles are substantially spherical.
11. A device according to any one of the preceding claims, wherein the device is extruded, and wherein the gas bubbles are formed by addition of gas during extrusion of the device.
12. A device according to any one of Claims 1 to 10, wherein the gas bubbles are formed by a chemical foaming agent.
13. A device according to any one of Claims 1 to 10, wherein the gas bubbles are provided by the incorporation of hollow microspheres into the plastics material.
14. A device according to any one of the preceding claims, wherein the device is tubular, wherein the plastics material is substantially transparent, and wherein the size and density of the bubbles is selected such as to enable material flowing along the device to be viewed by the eye.

15. A device according to any one of the preceding claims, wherein the plastics material is polyurethane.
16. An embryo replacement catheter comprising a flexible, hollow, extruded shaft of a substantially transparent plastics material, wherein the shaft includes gas bubbles through the thickness of its wall, wherein the density and size of the bubbles is selected to increase visibility of the catheter under ultrasound imaging whilst enabling an embryo within the catheter to be viewed by the eye, and wherein the bore of the catheter is smooth and uninterrupted by gas bubbles.
17. An embryo replacement catheter substantially as hereinbefore described with reference to the accompanying drawing.
18. A method of making a medico-surgical device comprising extruding a plastics material while incorporating a gas into the wall of the device such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.
19. A method of making a medico-surgical device comprising forming a wall of a plastics material containing a chemical foaming agent such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.

20. A method of making a medico-surgical device comprising forming a wall of a plastics material containing hollow microspheres such as to form gas bubbles through the major part of the thickness of the wall of the device sufficient to increase the visibility of the device under ultrasound observation.
21. A method of making an embryo replacement catheter substantially as hereinbefore described with reference to the accompanying drawing.
22. A device made by a method according to any one of Claims 18 to 21.
23. Any novel and inventive feature or combination of features as hereinbefore described.



INVESTOR IN PEOPLE

Application No: GB 0216145.3  
Claims searched: 1-22

Examiner: Dr. Simon Grand  
Date of search: 10 January 2003

## Patents Act 1977 : Search Report under Section 17

### Documents considered to be relevant:

Category	Relevant to claims	Identity of document and passage or figure of particular relevance	
X	1-3, 6-11, 13-15 and 18-21	EP 0386936 A1	(VANCE PRODUCTS INC.) See figs. and col.1 ll.17-31, col.3 ll.21-28 and col.5 ll.2-8
X	1-5 at least	DE 4014998 A1	(WOLF) See figs., col.3 ll.38-53 and WPI abstract acc. no.1991-341060/47
X	1 and 3	DE 3936162 A1	(SCHUBERT) See figs. and WPI abstract acc. no.1991-185943/25
X	18	WPI Abstract Accession No.1987-121289/17 of SU 1255450 A1 (KZEN-R KAZAN) See abstract	
A		EP 0624342 A1	(BECTON DICKINSON AND CO.) See figs.
A		WO 98/19713 A1	(STS BIOPOLYMERS) See whole document

### Categories:

X	Document indicating lack of novelty or inventive step	A	Document indicating technological background and/or state of the art
Y	Document indicating lack of inventive step if combined with one or more other documents of same category.	P	Document published on or after the declared priority date but before the filing date of this invention.
&	Member of the same patent family	E	Patent document published on or after, but with priority date earlier than, the filing date of this application.

### Field of Search:

Search of GB, EP, WO & US patent documents classified in the following areas of the UKC<sup>v</sup>:

--

Worldwide search of patent documents classified in the following areas of the IPC<sup>7</sup>:

A61B, A61L, A61M
------------------

The following online and other databases have been used in the preparation of this search report:

ONLINE :EPODOC, WPI, JAPIO
----------------------------



**THIS PAGE BLANK (USPTO)**